

FIG. 1

100

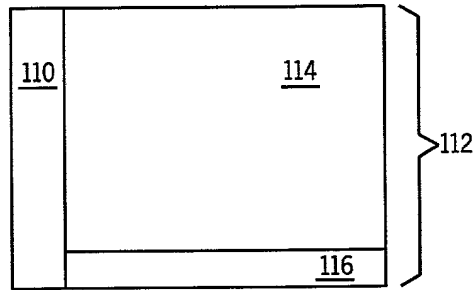


FIG. 2

100(a)



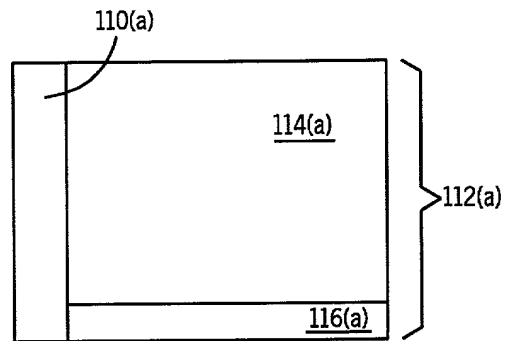


FIG. 3

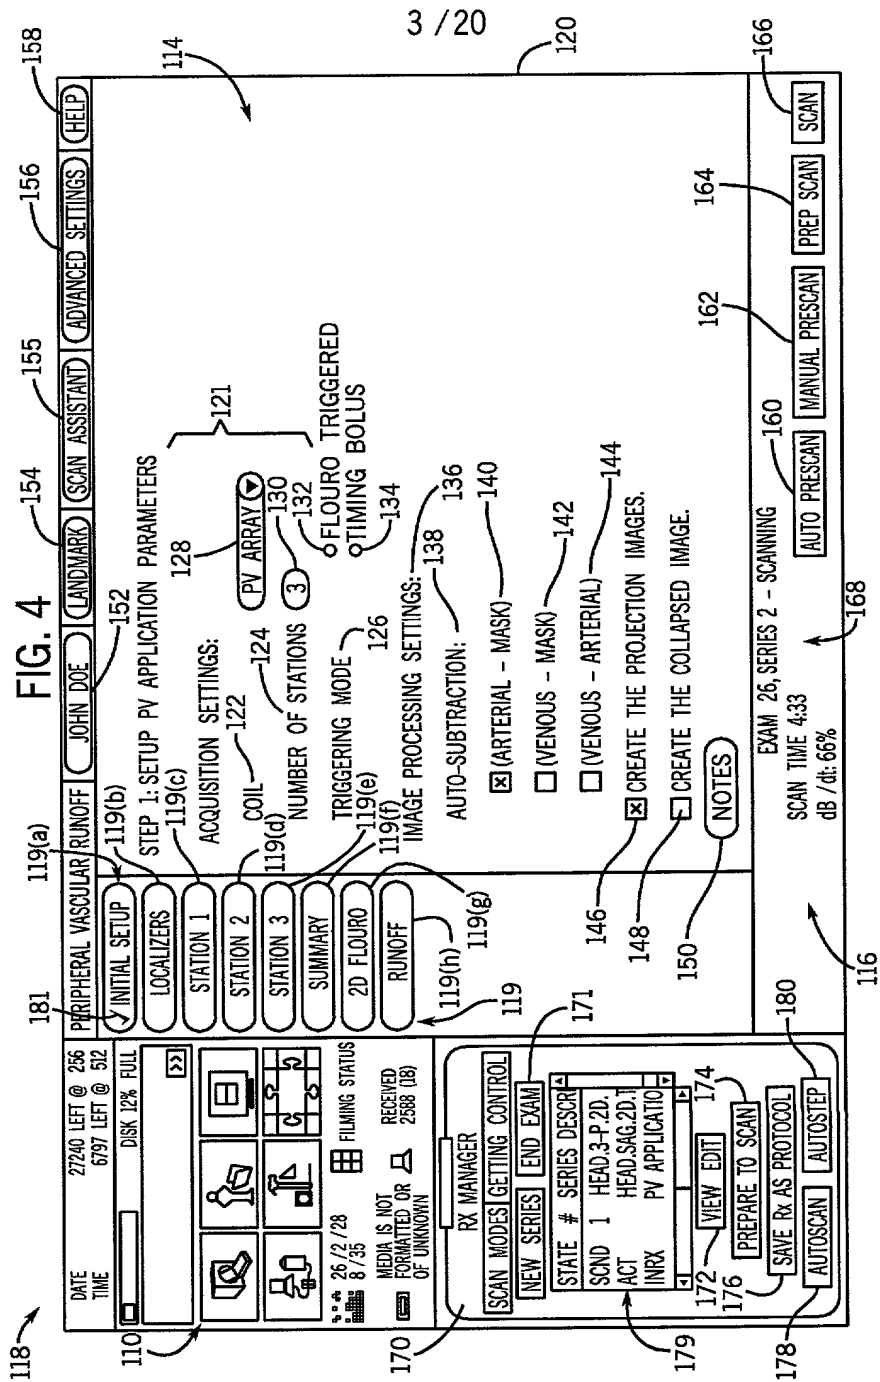

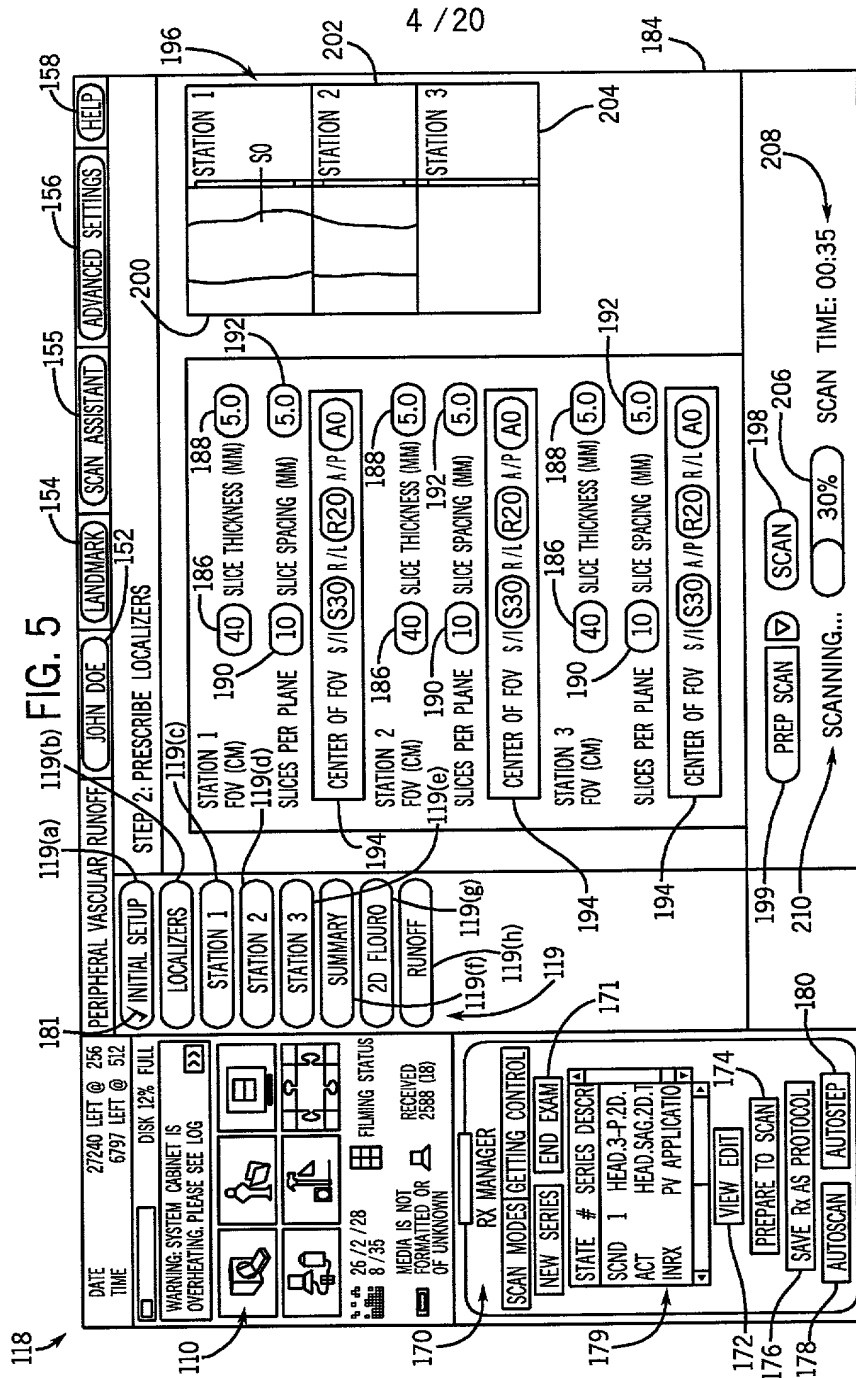


The form is titled "PATIENT INFORMATION" and contains the following fields and labels:

- ACCESSION NUMBER: 111222 (Label 214)
- PATIENT ID: 33-22-4444 (Label 216)
- PATIENT NAME: JOHN DOE (Label 218)
- BIRTHDATE: 9-22-1973 (Label 220)
- AGE: 27 (Label 226)
- SEX: M (Label 222)
- WEIGHT: 220 lb. (Label 220)
- Kg. (Label 224)
- RAD: SMITH (Label 228)
- REFER: TIMBO (Label 232)
- OPERATOR: WILSON (Label 230)
- STATUS: NONE (Label 234)
- EXAM DESCRIPTION: PV RUNOFF (Label 236)
- HISTORY: (Label 238)
- CLOSE button (Label 240)

The form is enclosed in a window frame with a title bar and a scroll bar on the right side. The label 212 points to the bottom of the window frame.

FIG. 6

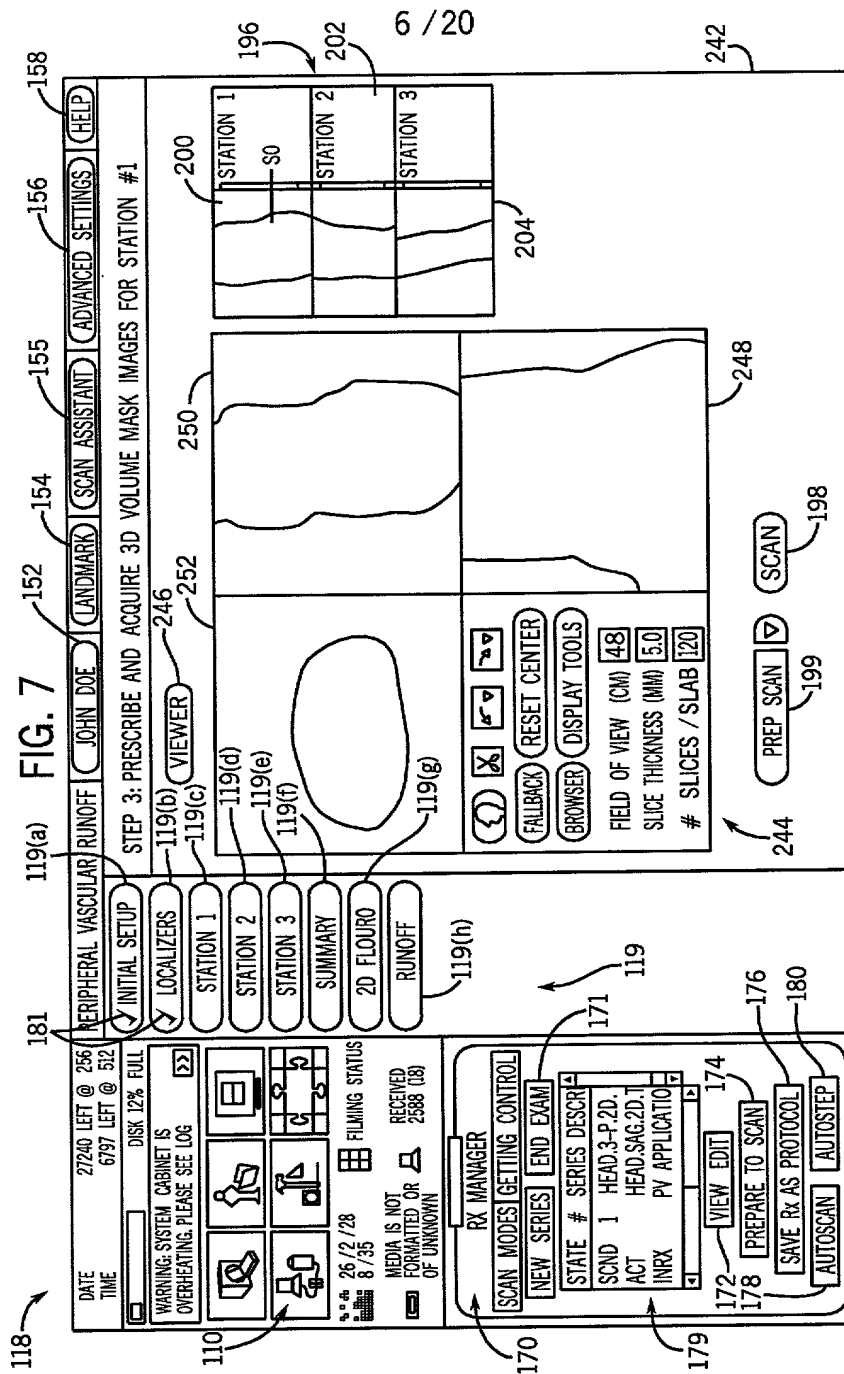

SCAN ASSISTANT

REQUESTED VALUE IS OUT OF RANGE.
FIELD OF VIEW (cm):50

DEFAULT TO MAXIMUM VALUE OF 48.


OR


ENTER A NEW VALUE BETWEEN
24 AND 48.


FIELD OF VIEW (cm): 48


ACCEPT CANCEL

FIG. 8

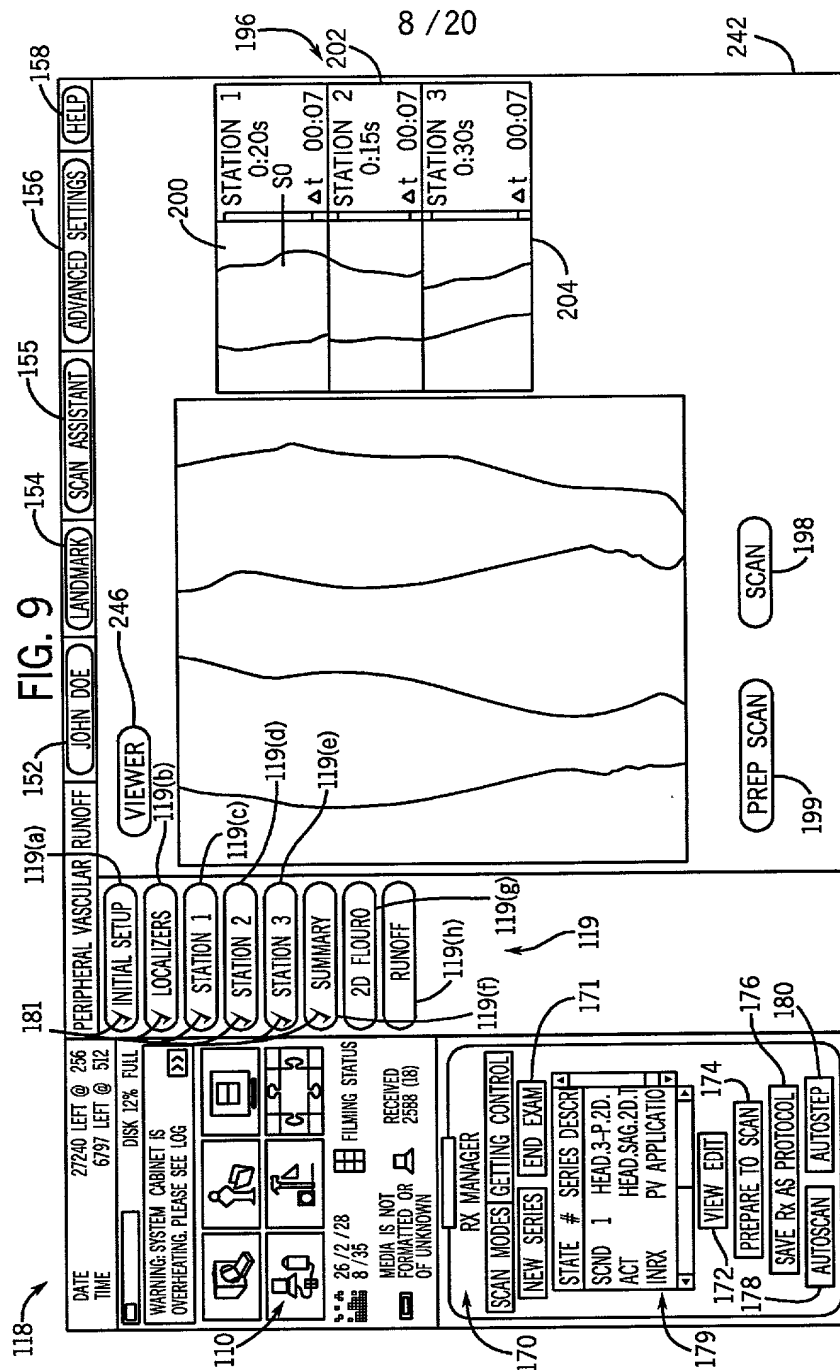

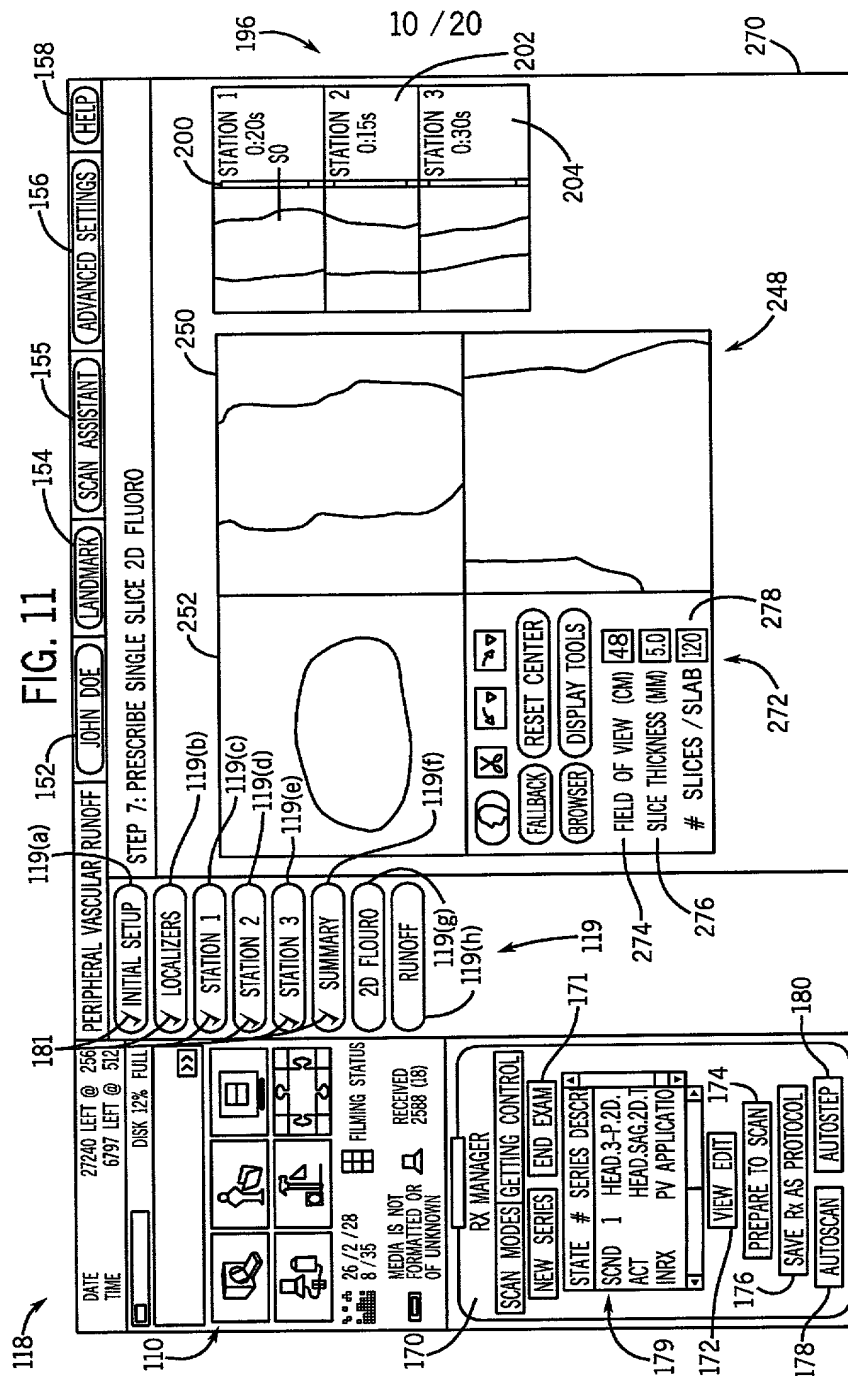

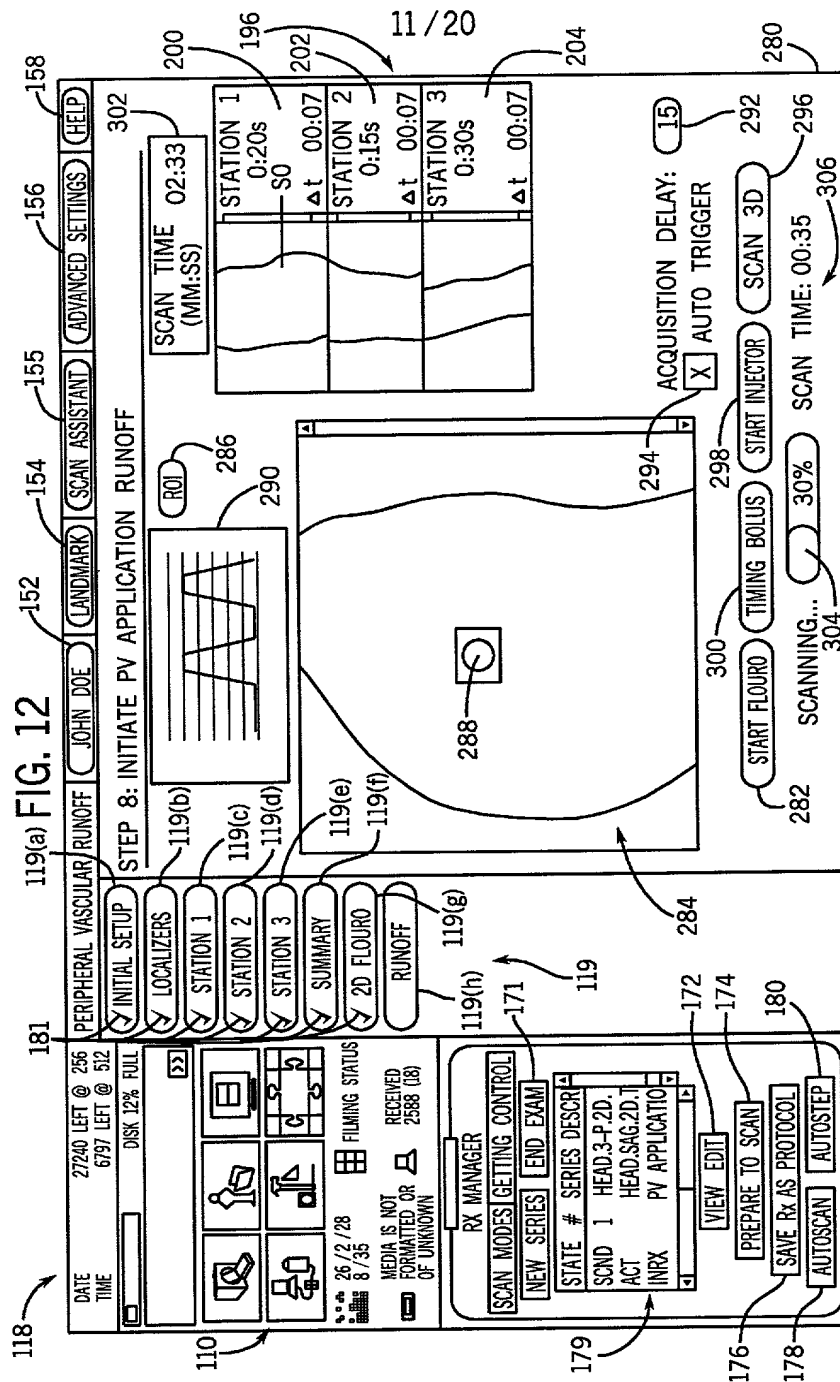

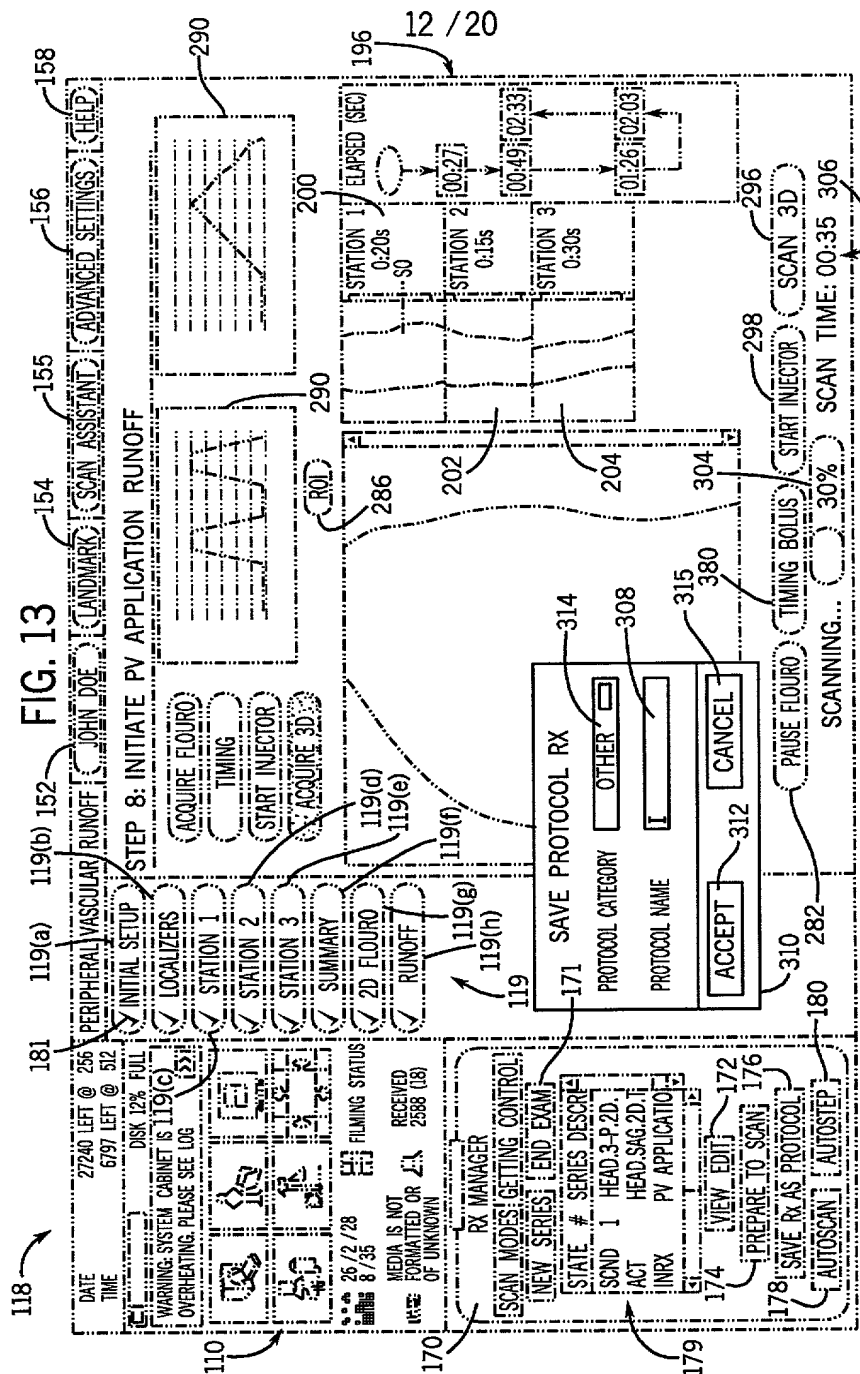

316

ADVANCED SETTINGS

INITIAL SETUP:

PATIENT INFORMATION:

PATIENT HEIGHT (cm) 150 324

PATIENT POSITION SUPINE

PATIENT ENTRY FEET FIRST

POST PROCESSING SETTINGS

☐ MAGNITUDE SUBTRACTION

☒ COMPLEX SUBTRACTION 318

☒ COLLAPSE PROJECTIONS

☐ PROJECTION INCREMENT 320

☐ 19 PROJECTIONS @ 20 DEG. INCREMENTS

☐ 30 PROJECTIONS @ 10 DEG. INCREMENTS

☐ USER SPECIFIED

☐ AXIS OF ROTATION X-AXIS 328

CLOSE 326

FIG. 14

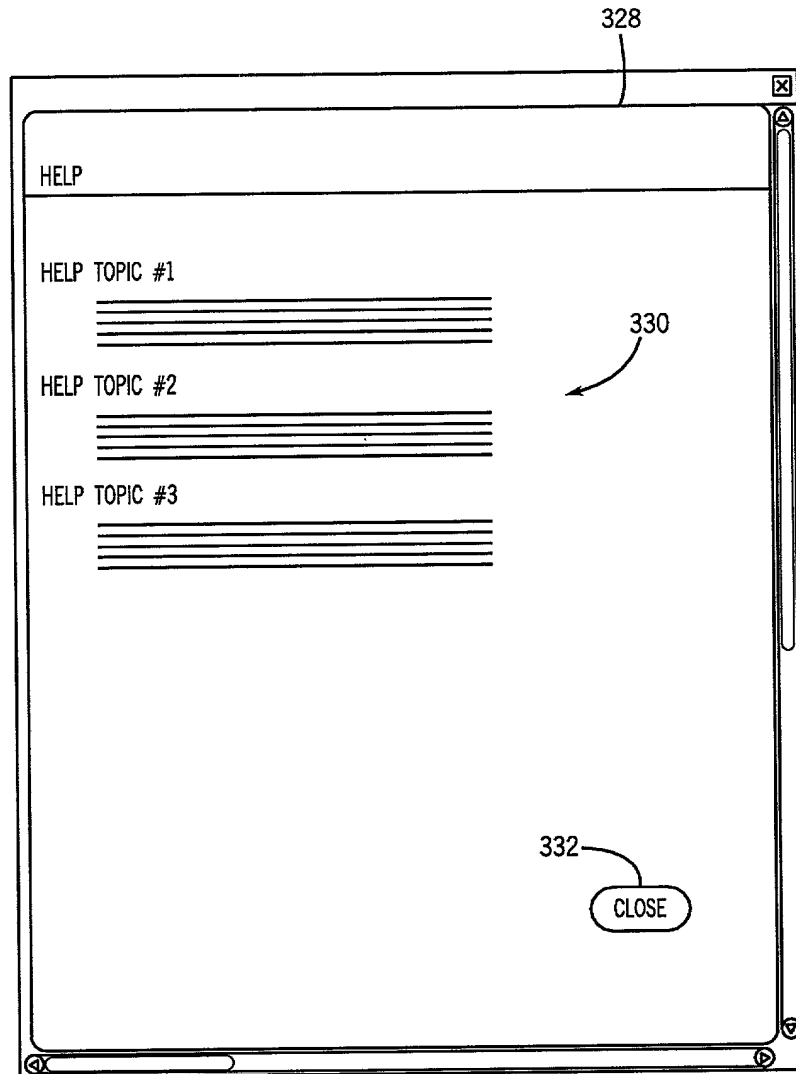


FIG. 15

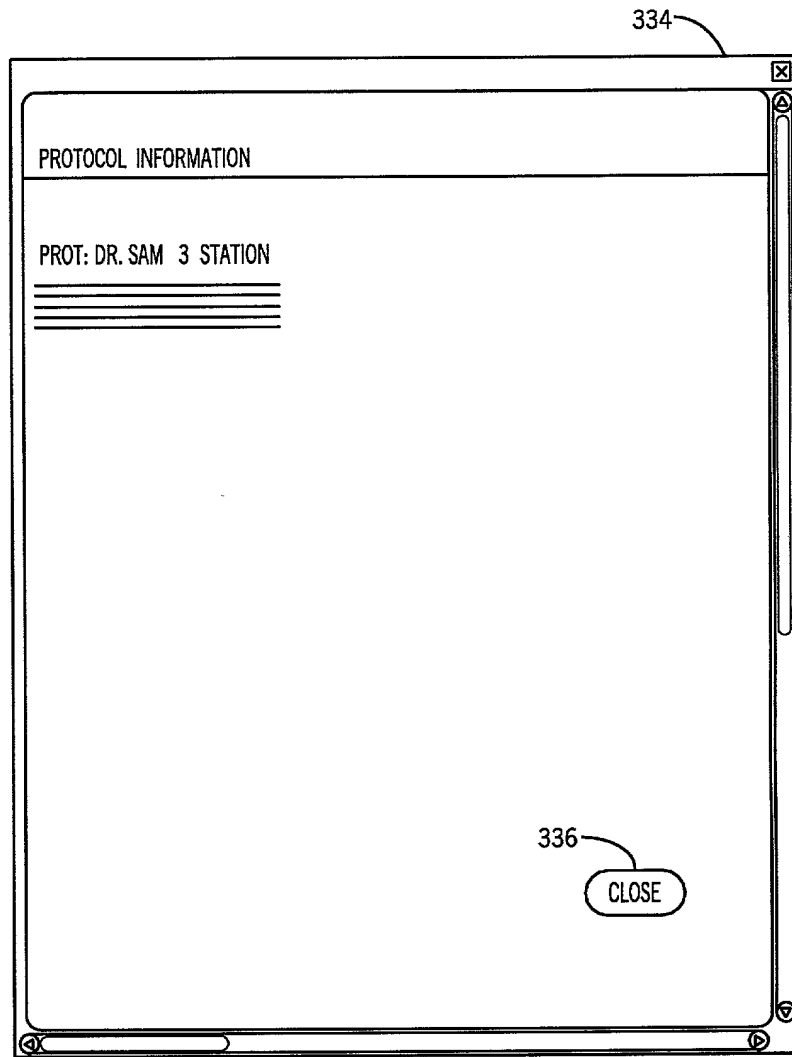


FIG. 16

